

FIG. 1

091200973 0722038

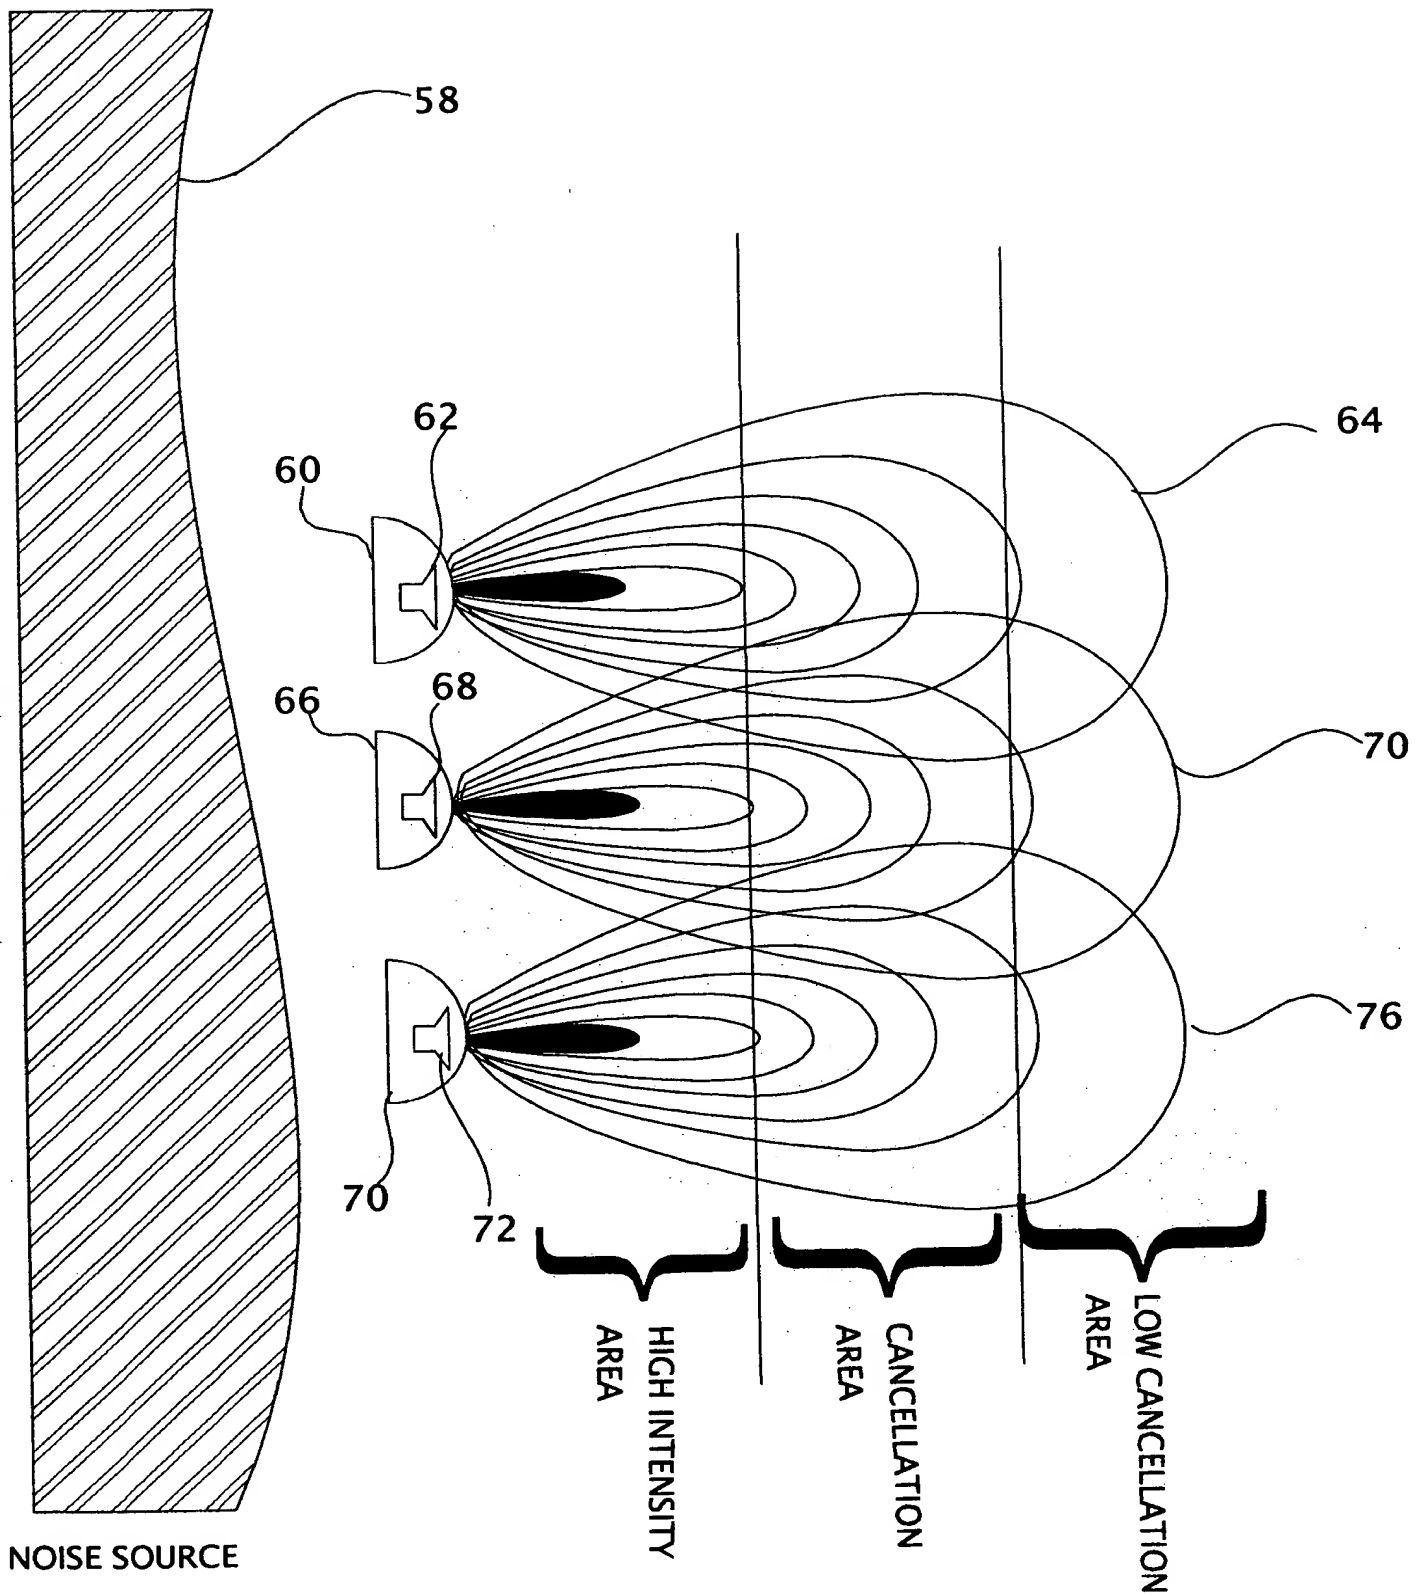


FIG. 3

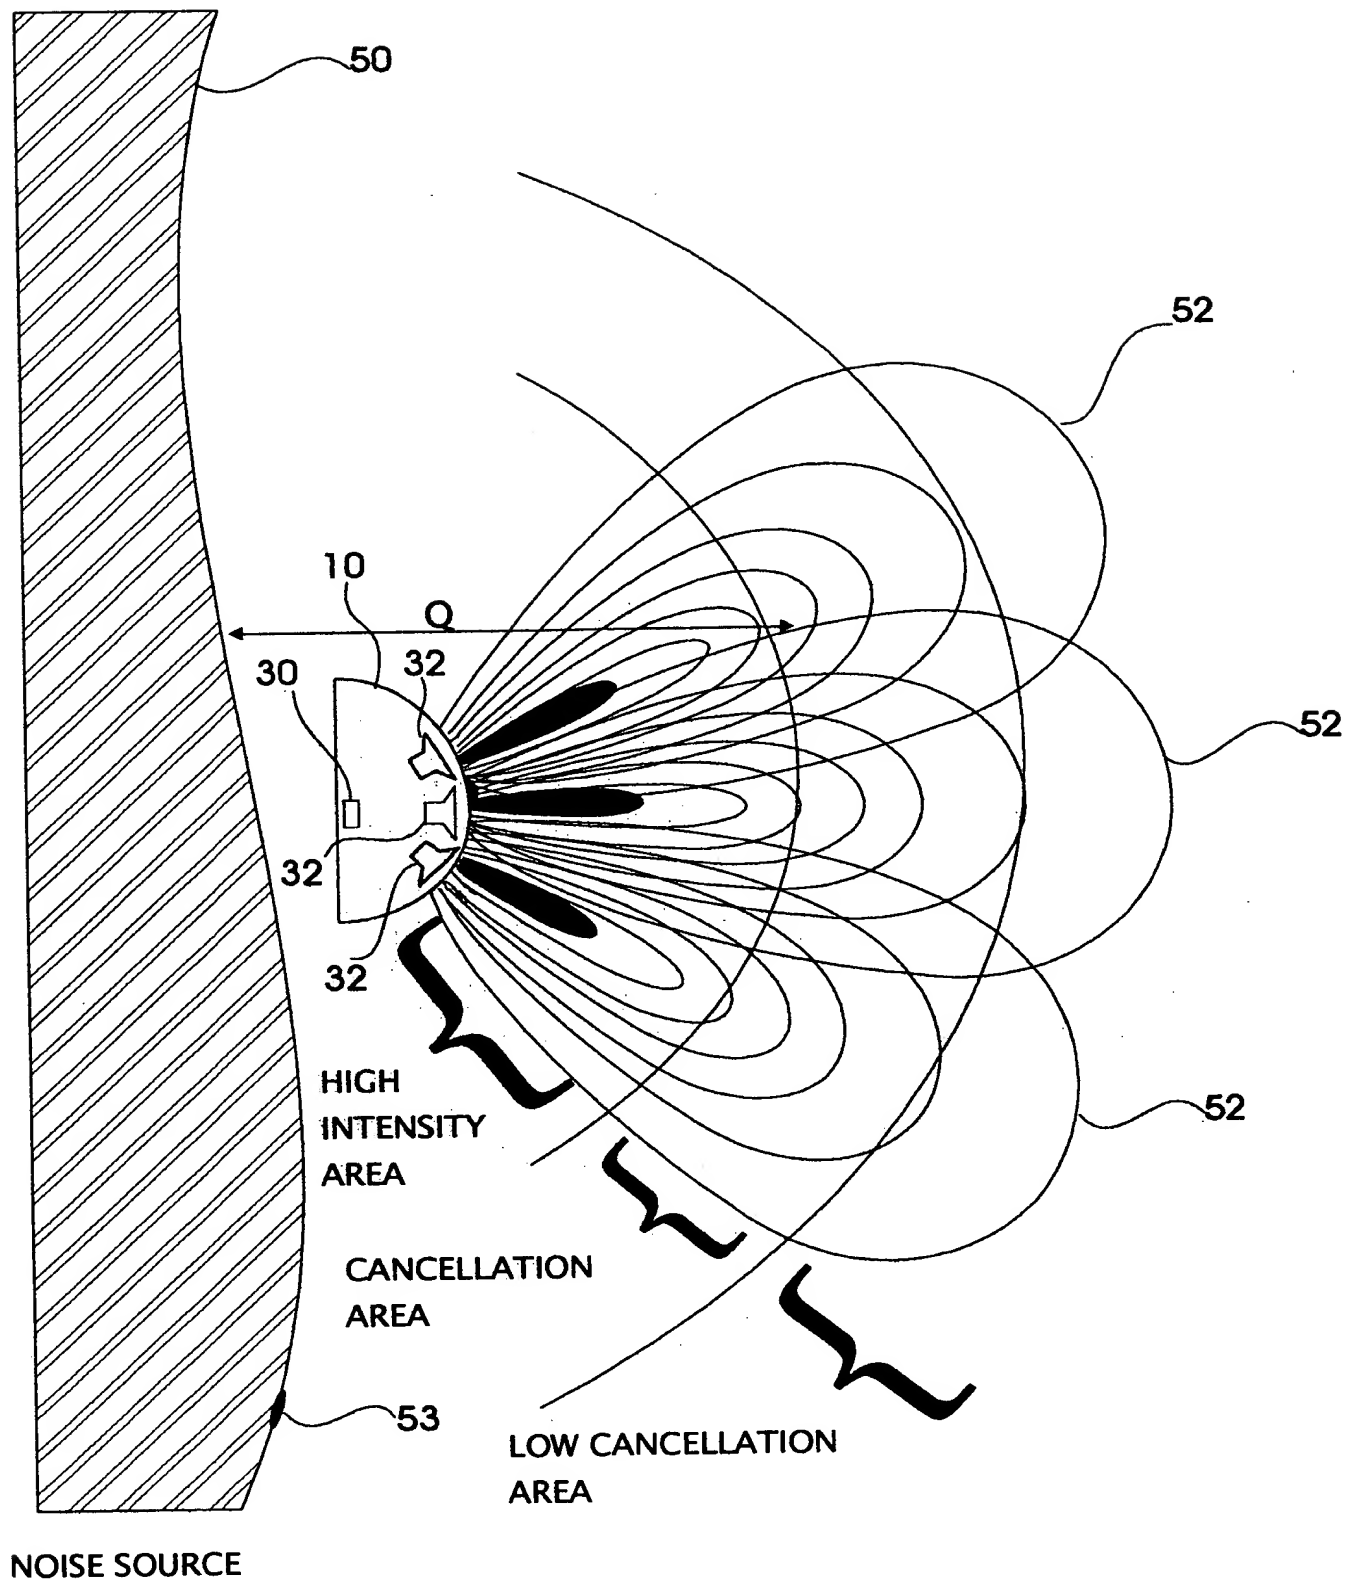


FIG. 2

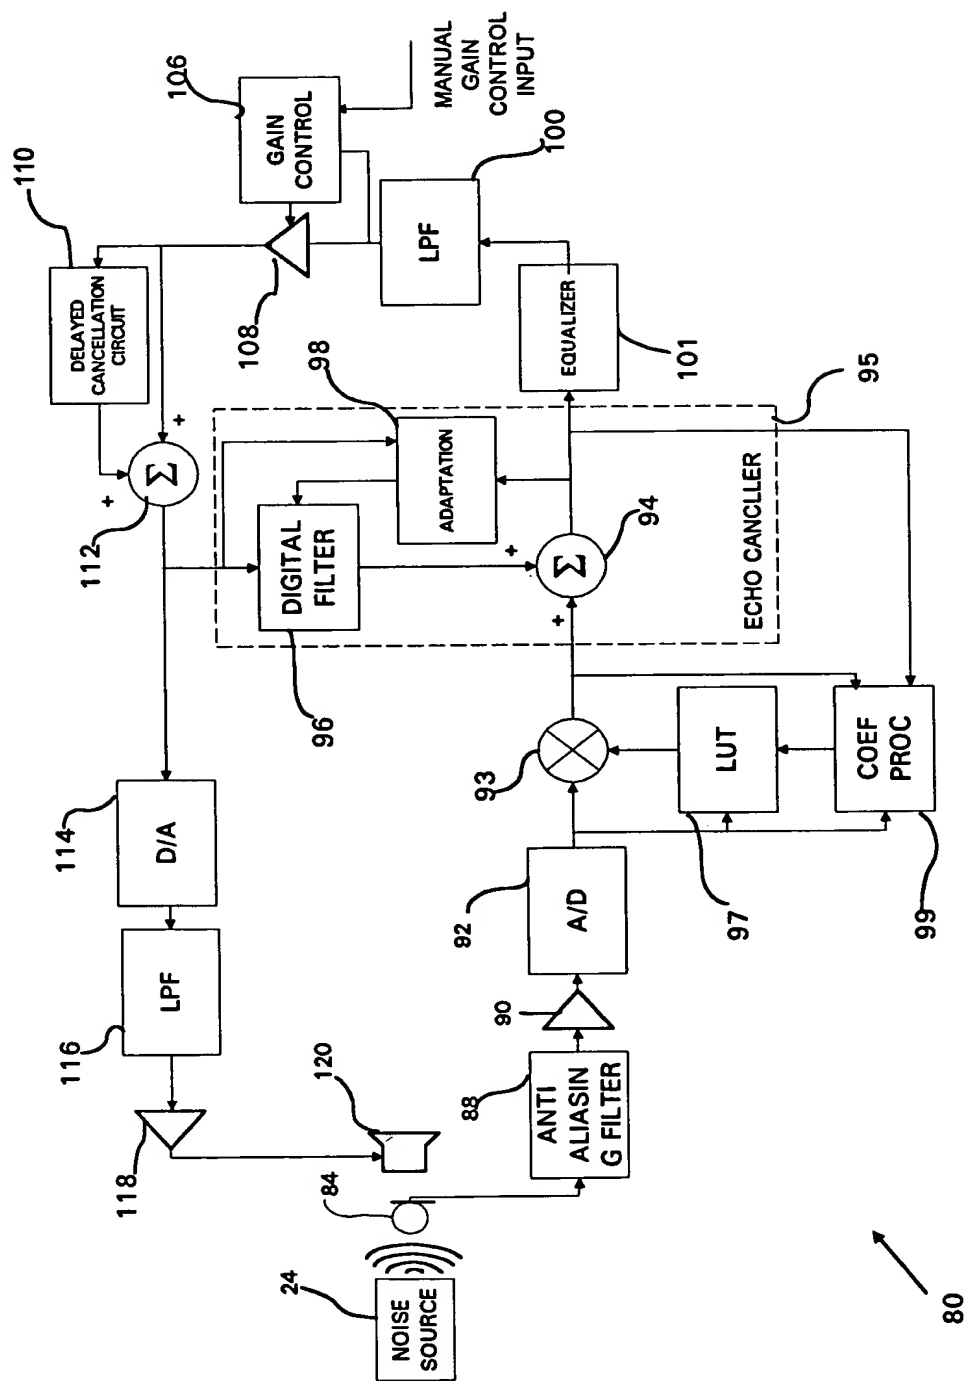


FIG. 4

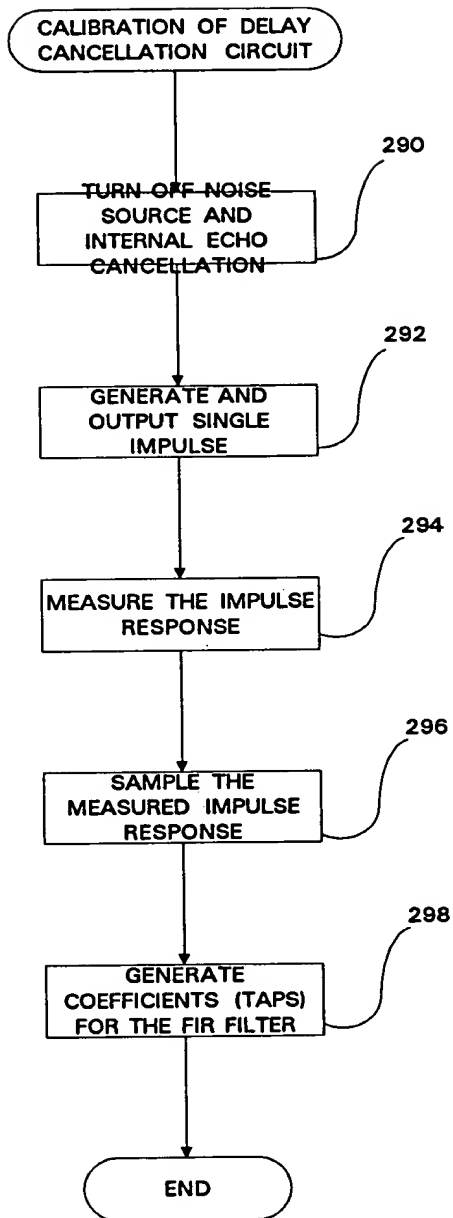
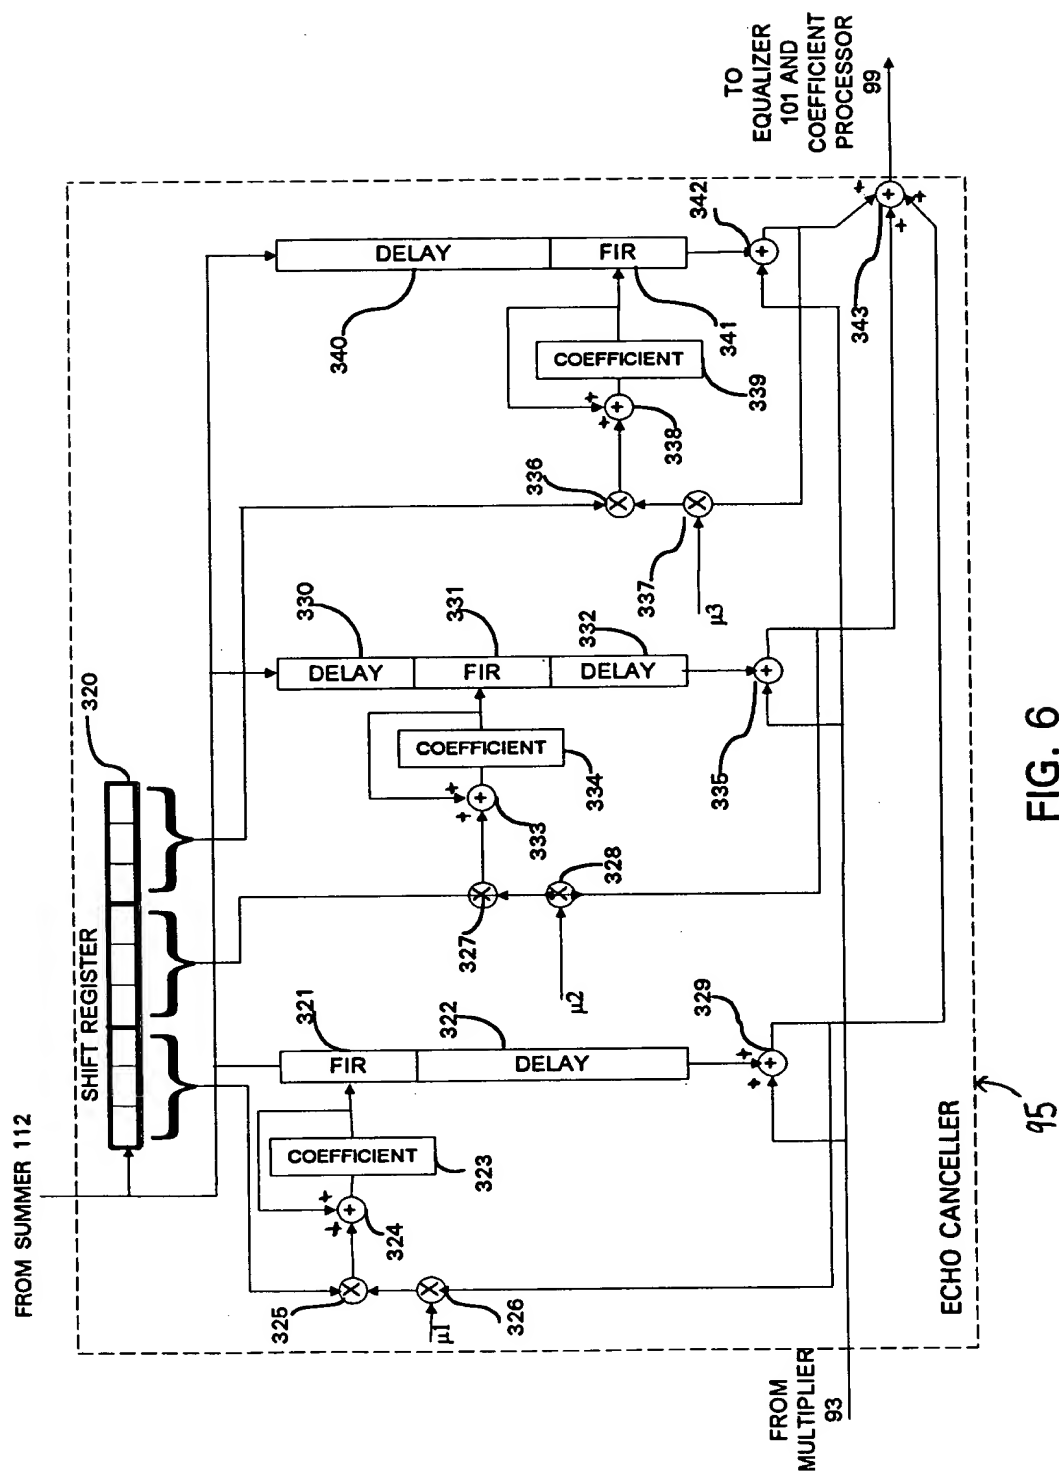


FIG. 5




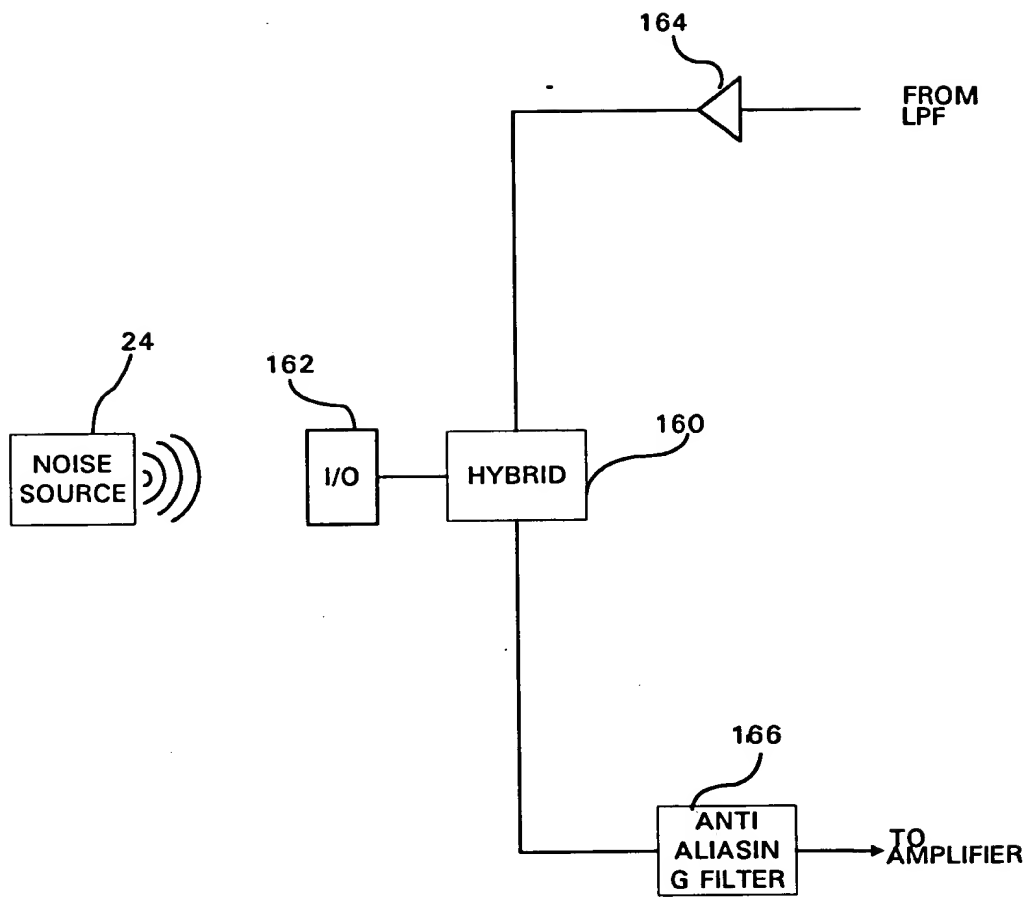


FIG . 7

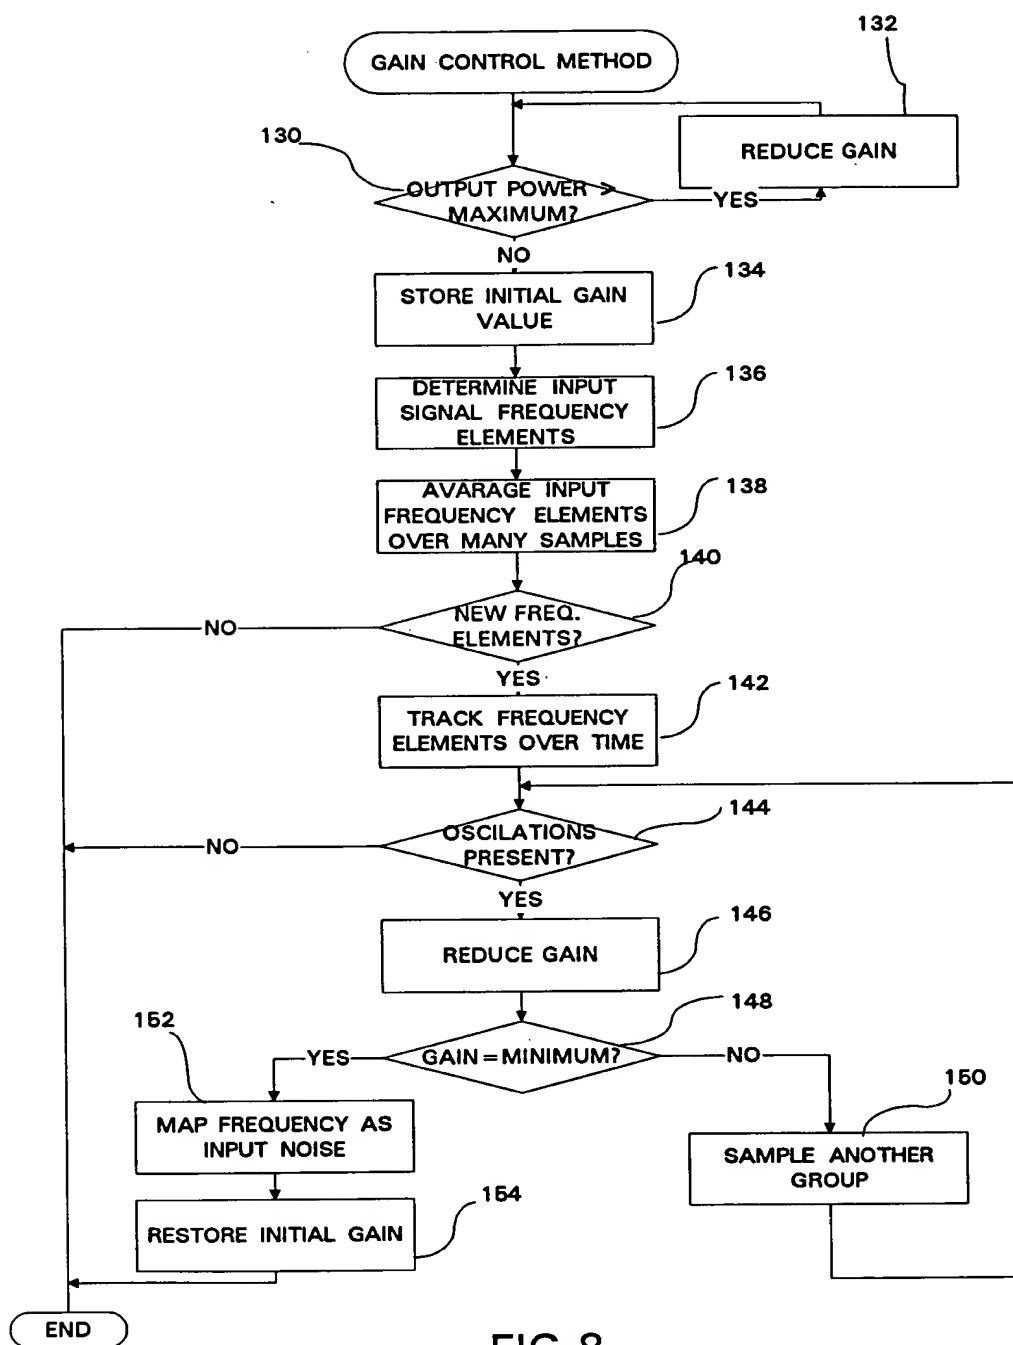

FIRST CALIBRATION METHOD
WITH ECHO CANCELLATION

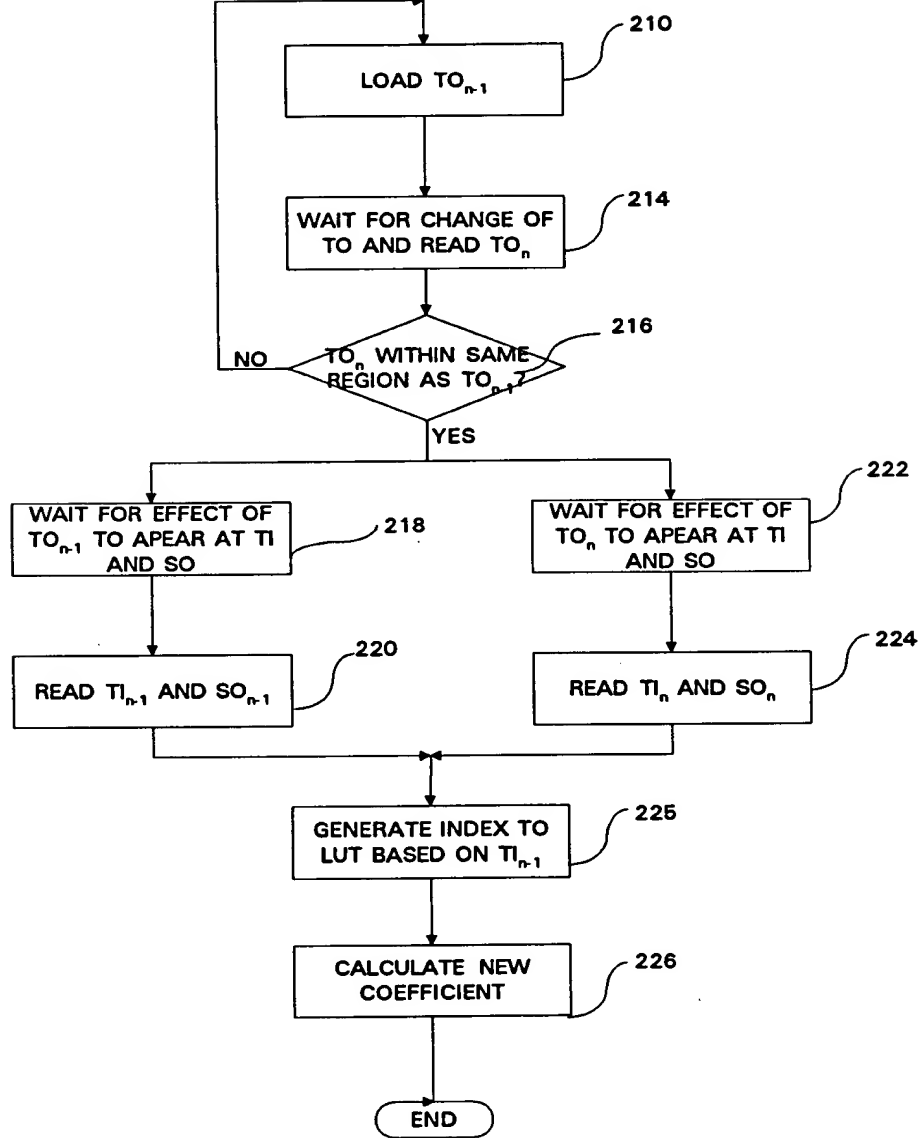


FIG. 9

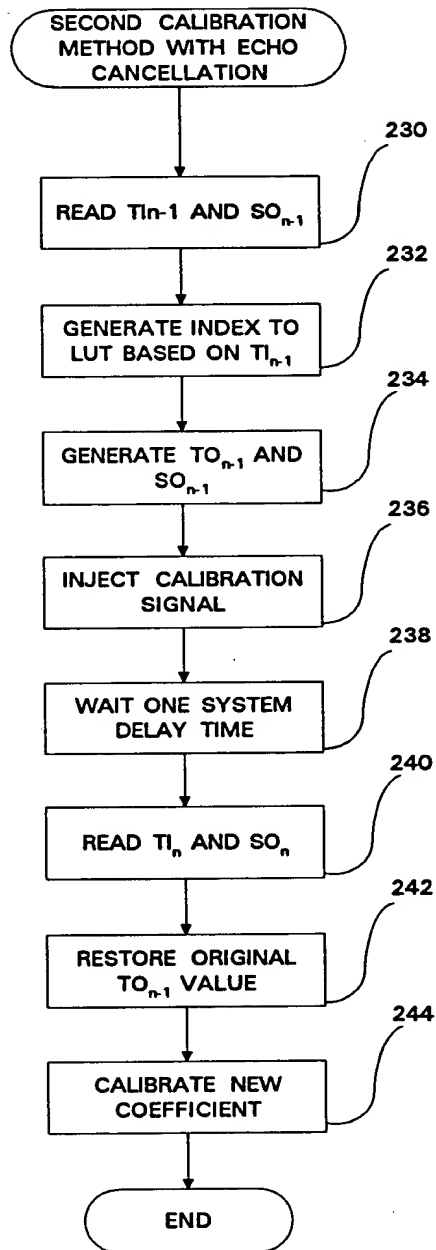


FIG. 10

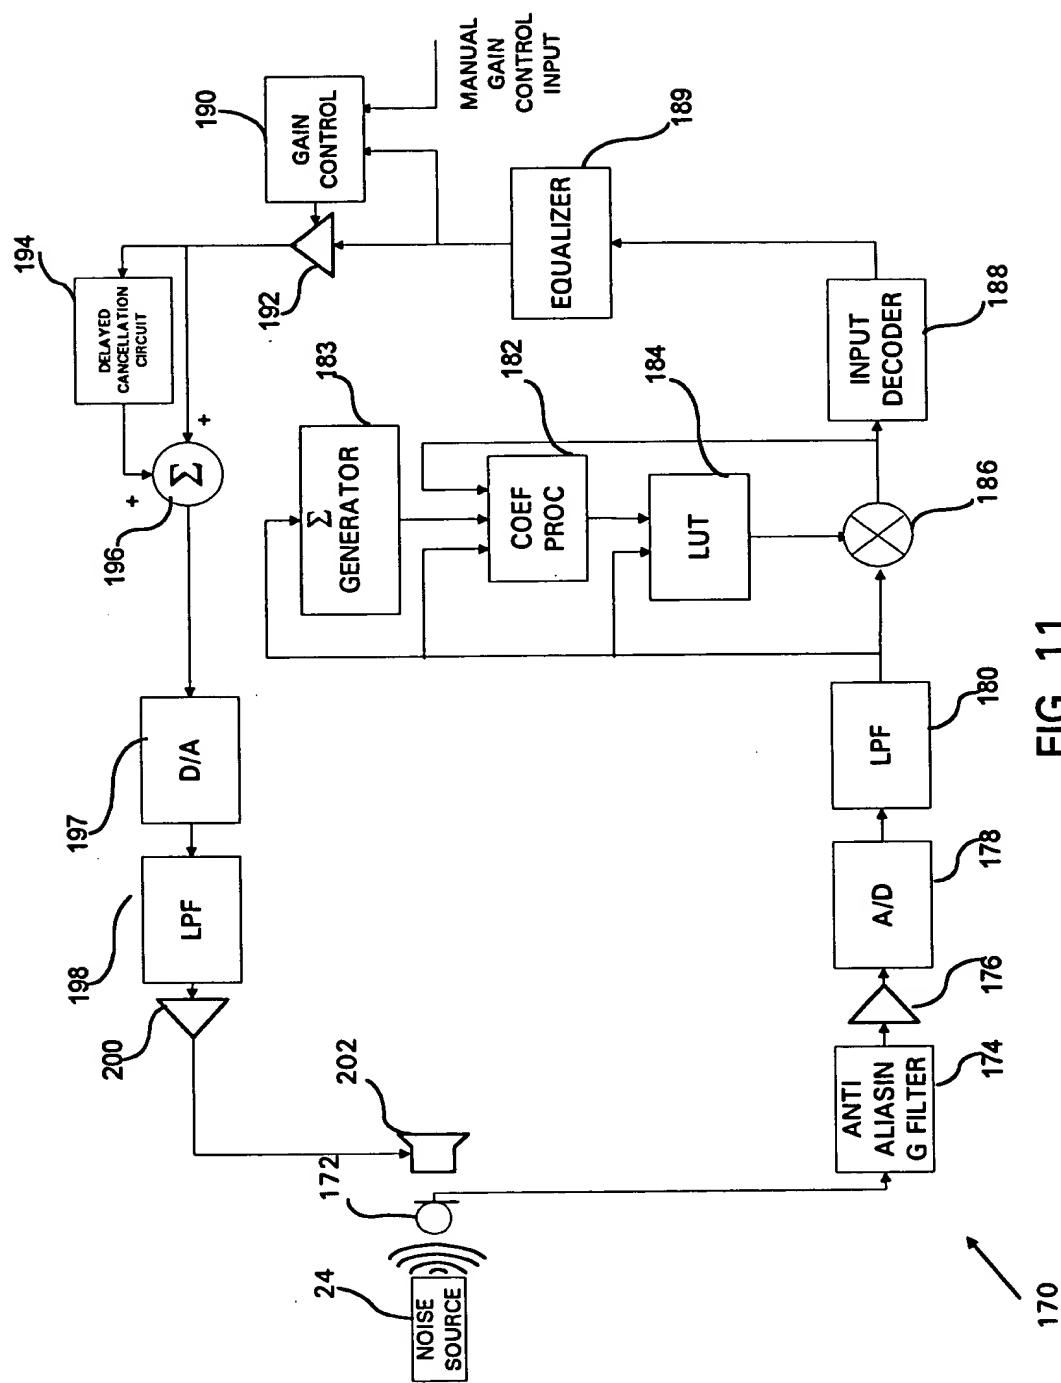


FIG. 11

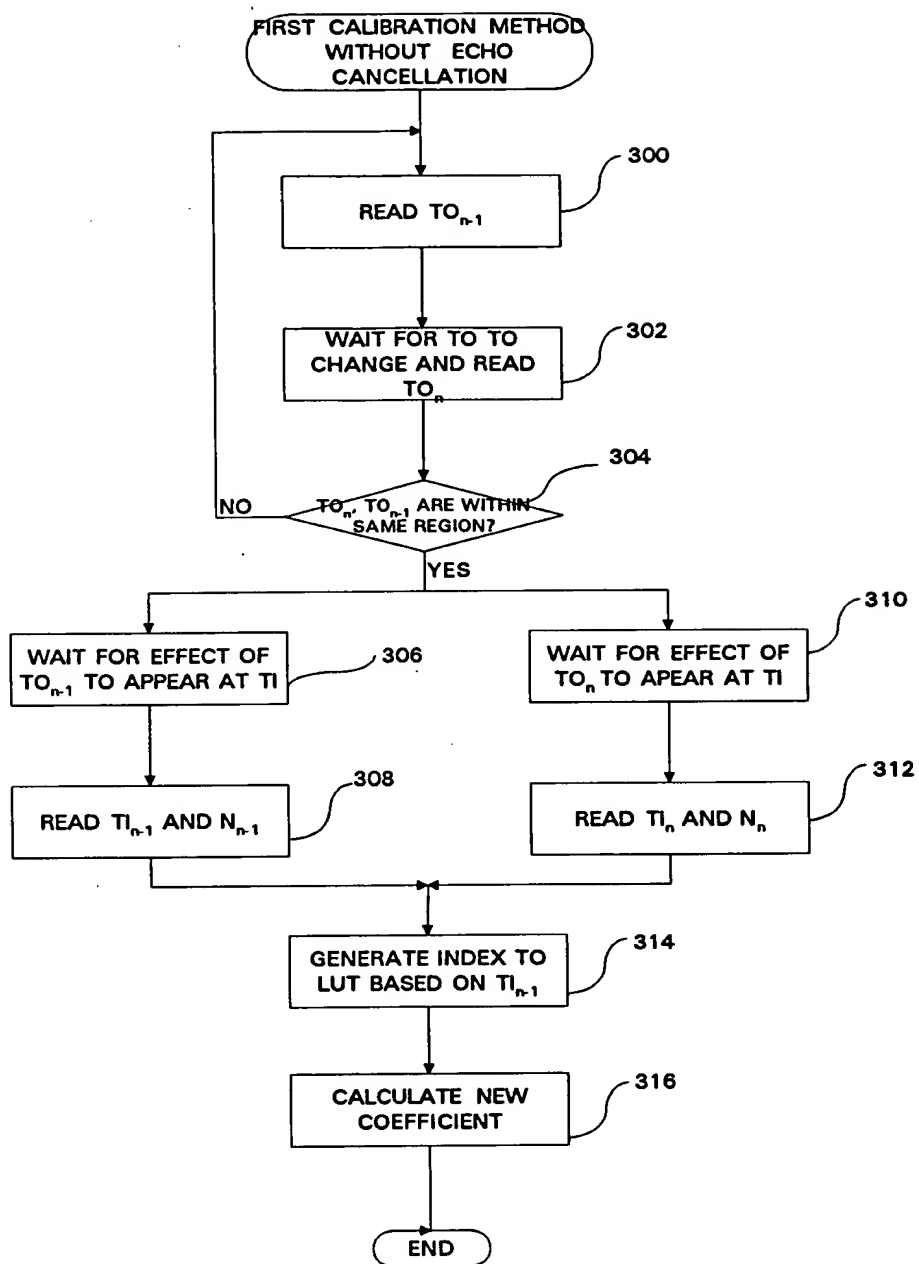


FIG. 12

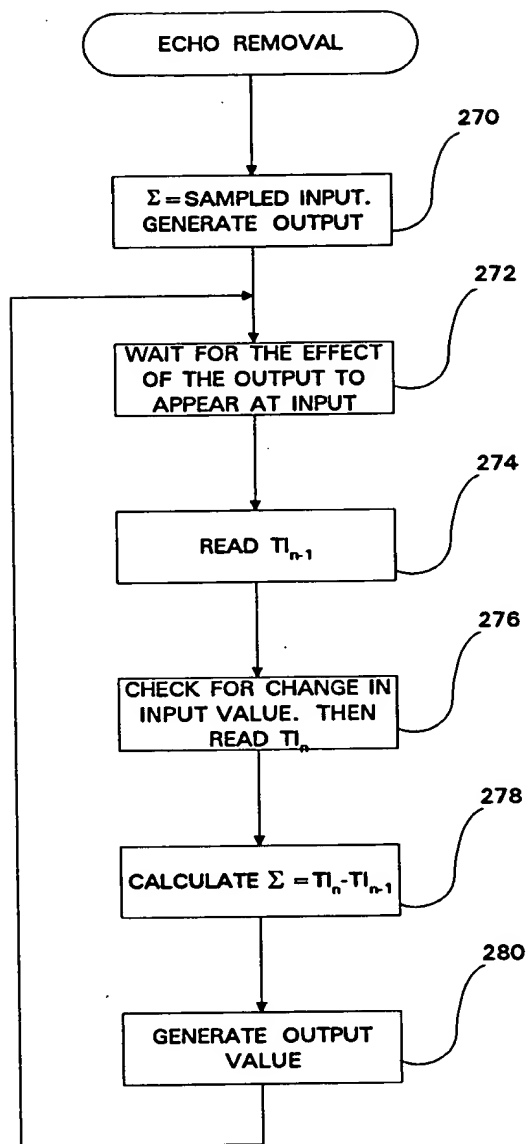


FIG. 13

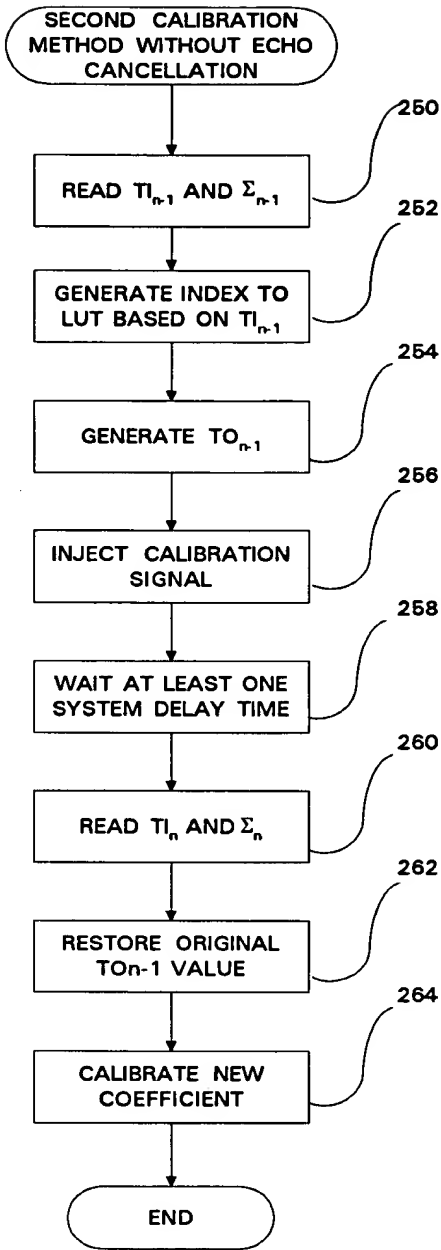


FIG. 14